TEST REPORT
Mikro Vision Glass Mop

Test item:	Domestic washing & bacteria pickup test
ISO standard:	6330:2021
Report no.:	DL-20241220-6
Test date:	17.10.2024
Issue date:	23.12.2024

Mikro Vision Glass Mop

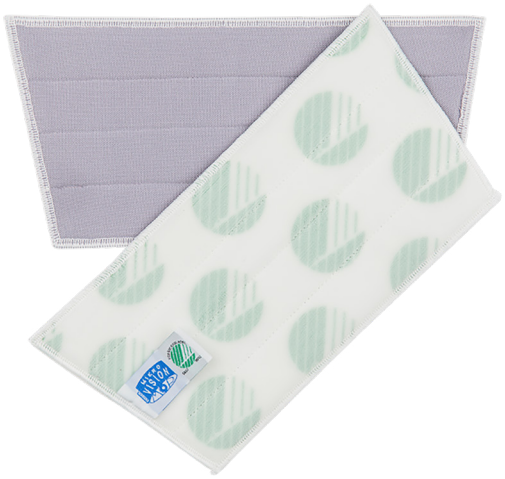

P-1200-G

For test result please see next page

Nordisk Microfiber
Kroghs Park 86
DK-5220 Odense SØ

65 98 20 40
info@nordiskmicrofiber.dk
www.nordiskmicrofiber.dk

TEST METHOD
Mikro Vision Glass Mop

Test conditions:

Test item		Pick-up rate (%)
Test bacteria		*Staphylococcus aureus* ATCC 6538
Test conditions	**Amount of water**	1 time of specimen weight
	Load weight	2 kg
	Surface	Vinyl tile (wax coated)
	Sliding range	30 cm
	Washing	Electrolux industry washing machine, 90 ° C Alkali detergent, 500 gange, pH=11
Pick-up rate (%)		$[(M_b - M_C) / M_b] \times 100$
		M_b = Average of the number of bacteria on the test surface before pick-up. (The amount of bacteria which was spread on the surface)
		M_c = Average of the number of bacteria on the test surface after pick-up. (The amount of bacteria on the surface after the wipe)

Illustration of the test method:

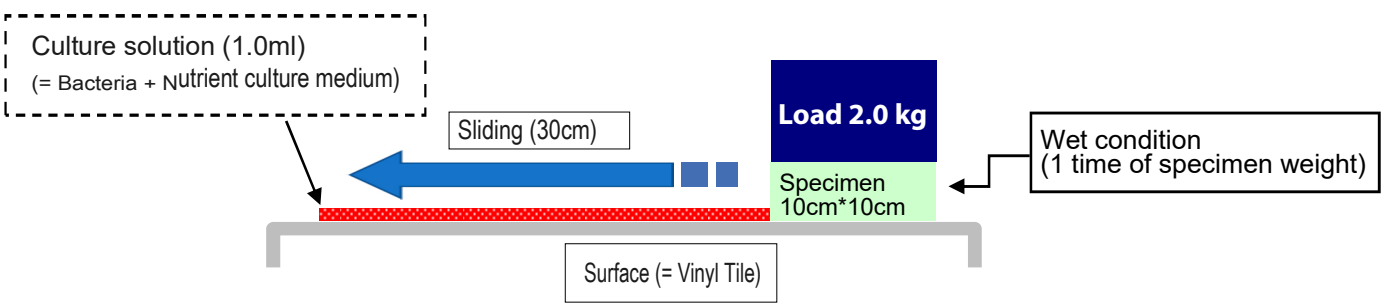

Nordisk Microfiber
Kroghs Park 86
DK-5220 Odense SØ

65 98 20 40
info@nordiskmicrofiber.dk
www.nordiskmicrofiber.dk

TEST RESULTS
Mikro Vision Glass Mop

Test results:

Test bacteria	*Staphylococcus aureus* ATCC 6538		
Test surface	Vinyl tile (wax coated)		
Specimen	**Mikro Vision Glass Mop (original)**	**Mikro Vision Glass Mop (After 300 washes 90 °C)**	**Mikro Vision Glass Mop (After 500 washes 90 °C)**
M_b	1,75 x 10^6 CFU	4,30 x 10^6 CFU	3,48 x 10^6 CFU
M_c	<50	<50	8,00 x 10^3
Bacteria pick-up rate (%)	99,9%	99,9%	97,7%

Before wipe:

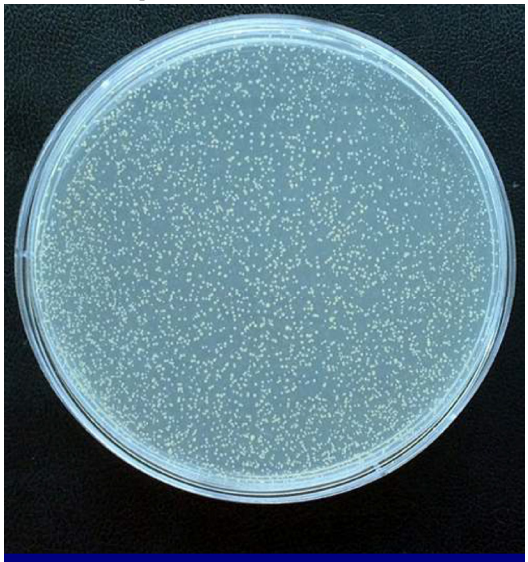

Bacteria Staphylococcus aureus

After wipe:

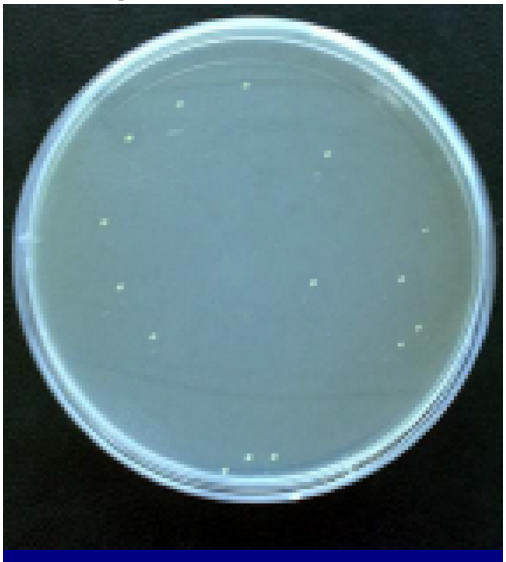

Bacteria Staphylococcus aureus

Nordisk Microfiber
Kroghs Park 86
DK-5220 Odense SØ

65 98 20 40
info@nordiskmicrofiber.dk
www.nordiskmicrofiber.dk

TEST RESULTS
Mikro Vision Glass Mop

Test item:	Domestic washing & bacteria pickup test
ISO standard:	6330:2021
Report no.:	DL-20241220-6
Test date:	17.10.2024
Issue date:	23.12.2024

CONCLUSION

Mikro Vision Glass Mop has a documented pick-up rate of microorganisms of min. 97,7%.

The test result is based on test with bacteria within the group of microorganisms, where viruses also are included as a part of this group because of their sizes.
When microfiber product's ability to pick up microorganisms is tested, the size of the test object is pivotal. Thus, it is not important whether the microorganism is a bacterium or a virus. Microfiber does not distinguish between the types of microorganisms when they pick them up. Microfiber's ability to pick up microorganisms varies from product to product.

The tests are always conducted with bacteria within the art of microorganisms because of two reasons:
1) Bacteria constitute the most extensive health risk because they multiply and evolve with time. Viruses disappear after a certain amount of hours.
2) Bacteria are more safe to use in tests and they are more accessible as test objects.

Nordisk Microfiber
Kroghs Park 86
DK-5220 Odense SØ

65 98 20 40
info@nordiskmicrofiber.dk
www.nordiskmicrofiber.dk

TEST REPORT
Mikro Vision Glass Mop

Test item:	Removal of dust and dirt
Report no.:	DL-20230714-8
Test date:	11.07.2023
Issue date:	14.07.223

Mikro Vision Glass Mop

P-1200-G

For test result please see next page

Nordisk Microfiber ApS
Agerhatten 27A
5220 Odense SØ

65 98 20 40
info@nordiskmicrofiber.dk
www.nordiskmicrofiber.dk

TEST RESULT
Mikro Vision Glass Mop

Test surface	Wooden floor			
Art. no.	P-1200-G Before washing		P-1200-G After washing (300 times)	
Condition	Dry	Damp	Dry	Damp
Turbidity before clean (Md)	1.60 NTU	0.96 NTU	2.01 NTU	1.62 NTU
Turbidity after clean (Mc)	47.71 NTU	50.08 NTU	28.1 NTU	25.97 NTU
Dust and dirt removal rate (%)	**96.6%**	**98.1%**	**92.8%**	**93.8%**

NTU = Nephelometric Turbidity Unit

The unit used to describe turbidity,
in other words the haziness of the water.
Nephelometric refers to the way the instrument,
a nephelometer, measures how much light is
scattered by suspended particles in the water.

The greater the scattering, the higher the turbidity.

Therefore, low NTU values indicate high water clarity,
while high NTU values indicate low water clarity. D

Nordisk Microfiber ApS
Agerhatten 27A
5220 Odense SØ

65 98 20 40
info@nordiskmicrofiber.dk
www.nordiskmicrofiber.dk

TEST METHOD
Mikro Vision Glass Mop

Test conditions:

Test surface	Wooden floor
Sliding range	10x30 cm
Washing	Household washing machine, 90 °C Weak alkali detergent 0.2% Washing times: 300 times

Calculation of the removal rate:

$$\text{Removal rate (\%)} = \frac{\text{Turbidity of before clean } \mathbf{(Md)} - \text{Turbidity of after clean } \mathbf{(Mc)}}{\text{Turbidity before clean } \mathbf{(Md)}} \times 100$$

Nordisk Microfiber ApS
Agerhatten 27A
5220 Odense SØ

65 98 20 40
info@nordiskmicrofiber.dk
www.nordiskmicrofiber.dk